

NSTX High Temperature Sensor Systems

H. W. Kugel^a, B. McCormack^a, R. Kaita^a, P. Goranson^b, L. Guttadora^a, R. Hatcher^a,
T. Holoman^a, D. Johnson^a, B. Nelson^b, C. Neumeyer^a, and A. L. Roquemore^a

^aPrinceton Plasma Physics Laboratory, Princeton University, Princeton NJ 08543-0451 USA

^bOak Ridge National Laboratory, Oak Ridge TN, 37831-8070 USA

ABSTRACT

The design of the more than 300 in-vessel sensor systems for the National Spherical Torus Experiment (NSTX) has encountered several challenging fusion reactor diagnostic issues involving high temperatures and space constraints. This has resulted in unique miniature, high temperature in-vessel sensor systems mounted in small spaces behind plasma facing armor tiles, and they are prototypical of possible high power reactor first-wall applications. In the Center Stack, Divertor, Passive Plate, and vessel wall regions, the small magnetic sensors, large magnetic sensors, flux loops, Rogowski Coils, thermocouples, and Langmuir Probes are qualified for 600 °C operation. This rating will accommodate both peak rear-face graphite tile temperatures during operations and the 350 °C bake-out conditions. Similar sensor systems including flux loops, on other vacuum vessel regions are qualified for 350 °C operation. Cabling from the sensors embedded in the graphite tiles follows narrow routes to exit the vessel. The detailed sensor design and installation methods of these diagnostic systems developed for high-powered ST operation are discussed.

I. INTRODUCTION

The National Spherical Torus Experiment (NSTX) has unique high temperature in-vessel sensor systems mounted in small spaces behind plasma facing armor tiles prototypical of possible high power reactor first-wall applications. NSTX is designed to investigate the physics of Spherical Tori (ST) in a device that can produce non-inductively sustained high- β discharges in the 1 MA regime and to explore approaches toward a small, economic, high power density Volume Neutron Source (VNS) and an ST reactor core.[1] Fig.1 shows a partial schematic cross section of the NSTX. The device capabilities include $R = 0.85$ m, $a = 0.68$ m, $I_p = 1$ MA, $B_T = 0.3$ T, $k = 2.0$, $R/a = 1.27$ and a 5 sec maximum pulse length. The start-up will employ Ohmic Heating (OH), Electron Cyclotron Preionization (ECP), and Co-Axial Helicity Injection (CHI). Wall stabilization will be provided by close-fitting,

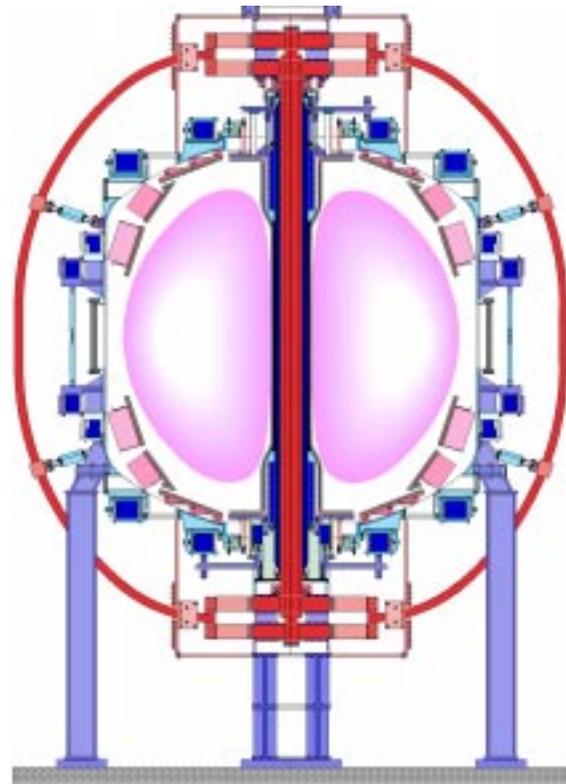


Fig.1. Partial schematic cross section of NSTX. The diameter of the Center Stack at the midplane is 38 cm. The outer diameter of the vessel at the midplane is 341 cm.

high conducting 2.5 cm thick copper Passive Stabilizer Plates. Auxiliary Heating will be provided by CHI, 6 MW of High Harmonic Fast Wave (HHFW) Radio Frequency heating, and 5 MW of Neutral beam Injection (NBI). Profile control will be studied using the HHFW, CHI, and NBI systems. The device has Divertors and allows for single-null, double null, and inner wall limited discharges. High power densities are expected on the Center Stack and Divertor. During high power, 5 sec long discharges applied every 300 sec, e.g., the Center Stack tiles will receive incident power densities of 7 MW/m² and reach peak front face temperatures of about 1200 °C. The temper-

Location	Sensor	No.	Install (ed)
CS-air	Flux Loops	17	2/15/99
	Plasma Rogowski Coils	2	2/15/99
	Thermocouples	24	2/15/99
	Subtotal	43	
CS-vac	Thermocouples	32	6/1/99
	Langmuir probe	14	6/1/99
	Bz Coils	21	6/1/99
	2D Coils	12	6/1/99
	Halo Rogowski Coils	4	6/1/99
	Subtotal	83	
Otr Div	Flux Loop Tubes	6	6/1/99
	Thermocouples	20	6/1/99
	Langmuir probe	10	6/1/99
	2D Coils	14	6/1/99
	Neutral Pressure Gauge	1	2/99
	Subtotal	51	
Sec PP	Flux Loop Tubes	8	6/1/99
	Thermocouples	8	2/00
	Langmuir probe	0	CY01
	2D Coils	12	2/00
	Eddy Current Rog Coils	8	2/00
	Large 1D Coils	12	2/00
	Subtotal	48	
Pri PP	Flux Loop Tubes	8	6/1/99
	Thermocouples	8	2/00
	Langmuir probe	0	CY01
	1D Coils	8	2/00
	2D Coils	16	2/00
	Large 2D Coils	12	2/00
	Eddy Current Rog Coils	8	6/1/99
	Subtotal	60	
Otr In-Ves	Flux Loop Tubes	4	6/1/99
	Thermocouples	12	2/00
	Large 2D Coils	18	2/00
	Subtotal	34	
Ex-Vessel	on Vessel Flux Loops	12	8/1/99
	on PF Coil Flux loops	9	8/1/99
	Subtotal	21	
Total		340	

Table 1. Vessel Sensor Summary. CS-air (Center Stack Air-side), CS-vac (Center Stack,Vacuum-side), Otr Div (Outer Divertor), Sec PP (Secondary Passive Plates), Pri PP (Primary Passive Plates), Otr In-Ves (Outer Vessel interior Wall), Ex-Vessel (Vessel air side).

-atures at the end of the cool-down after multiple pulses will be about 540 °C. Analysis indicates that Divertor front face temperatures could exceed 1200 °C design limit. Sweeping the strike-points could reduce the peak temperatures. Wall conditioning will be performed with Glow Discharge Cleaning, Bake-out to 350 °C, and wall coatings. During Bake-out, the tiles will be maintained at 350 °C, the view-

ports and the signal cable feed through connectors and most of the vessel will be maintained at 150 °C. The sensors mounted in the Center stack tiles are qualified for 600 °C operation. All other in-vessel tile sensors are qualified for 350 °C Bake-out temperatures.

II. OVERVIEW OF IN-VESSEL SENSORS

Over 300 sensors either have been installed or are scheduled for installation inside the vacuum vessel or on outside of the vessel subject to bakeout temperatures. All sensor fabrication materials and signal cabling are qualified for 600 °C temperatures, and for operation in the NSTX vacuum chamber at base pressures in the 10^{-8} torr range. Table 1 gives a partial list of these sensors and their installation status. These include small 1-D Mirnov coils, small 2-D Mirnov coils, large 1-D Mirnov coils, interior Flux Loops, Halo current and Eddy current Rogowski coils, thermocouples, and Langmuir Probes. Outside the vacuum vessel, on the air-side of the Center Stack, are mounted Flux Loops, thermocouples and plasma current Rogowski coils. In addition, there are Flux Loops on the air-side of the vessel, and a Flux Loop mounted on each outer PF coil.

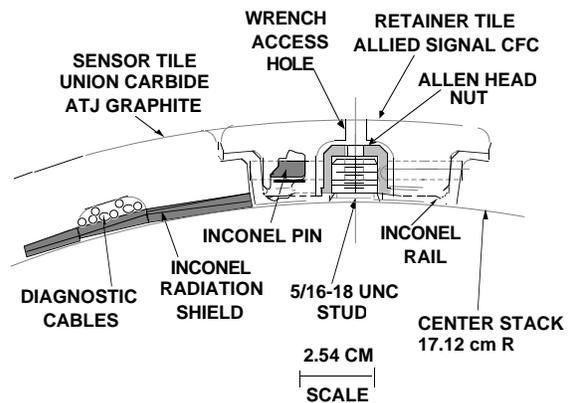


Fig.2. Partial schematic of 1.27 cm (0.5") thick Center Stack Sensor Tile and Retainer Tile assemblies.

The design of the in-vessel sensor systems encountered the requirements of high temperatures, due to Bakeout and the expected thermal loads, as well as the small space available for embedding in the tiles, and in addition, the small spaces available for the exiting signal cables. The wall armor on the Center Stack consists of 1.27 cm (0.5") thick tiles composed of alternating columns of Allied Signal C-C Composite tiles and Union Carbide ATJ graphite tiles fastened to the Inconel Center Stack with bolts (refer to Fig.2). All sensors on the Center Stack are embedded on the back-side of the 1.27 cm thick tiles and are separated from the Center stack by a 0.15 cm thick Inconel radiation shield. Each sensor tile has a 1.27 cm wide by 0.317 cm (0.5" x 0.125") deep vertical channel on the backside for the exiting signal cables.

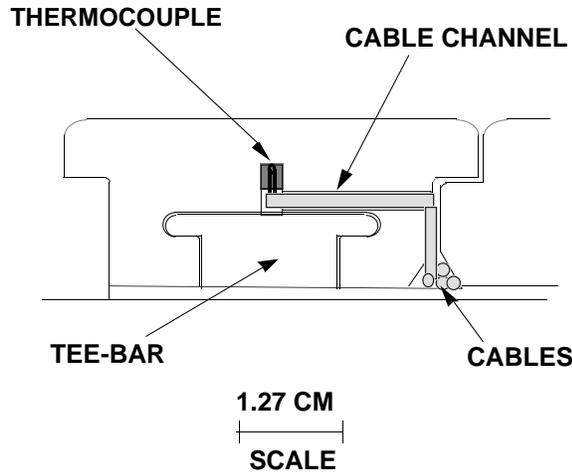


Fig.3. Partial schematic of typical Divertor or Passive Plate graphite sensor tile design showing thermocouple.

The tiles cladding the Divertor and Passive Plate Stabilizer are 2.54 cm (1") thick Union Carbide ATJ graphite, and are mounted to the copper backing plate with Tee-bars with Grafoil, a thermal conductive gasket, between the tiles and the copper. All sensors cladding the Divertors and Passive Plates are embedded in the backside of the tiles mounted above the Tee-bars. These tiles are chamfered on the edge to allow an exit channel for the signal cables.

III. SIGNAL CABLES

The signal cables must be vacuum compatible with vessel base pressure in the low 10^{-8} torr range, qualified for 600 °C service (in the most severe case), and allow high quality transmission of low level signals in the presence of rapidly varying magnetic fields, and high electromagnetic interference. In principle, a twisted pair of conductors, insulated with a suitable silicon based fiber, and protected with a 304-SS braid can meet these requirements. However, the physics requirement to minimize the diameter of the Center Stack results in tiles of minimal thickness with very small cable exit channels (1.27 cm x 0.317 cm) on the rear face of the tiles (Fig.2). This small exit channel must accommodate not only the signal cable exiting a particular tile but also signal cables from other tiles exiting via the same channel. This requirement eliminated typical commercially available 304-SS braided high temperature (650 °C) twisted pair wire. Thermo Electric Corp. Q-Glass insulated AWG No. 24 twisted non-jacketed copper-copper (Q/TW-24-) was selected for the sensor cable, and the Type-K version (Q/TW-24-) for the thermocouple wire [2]. This is a twisted-pair, No. 24 gauge wire (0.051 cm dia.) with a nominal outer width of about 0.2 cm. This wire is typically available with a polyester silicone enamel saturant for color coding and providing mechanical stability during installation. In order to make the wire vacuum compatible at high temperature, it was air baked at 600 °C for 4 hours.

Testing of wire prepared in this manner for out-gassing in high vacuum at temperatures up to 600 °C using a Residual Gas Analyzer (RGA) indicated that it was suitable for operation in the NSTX environment. However, this procedure made the quartz-based jacket more fragile, and hence, after air-baking the wire was coated with a dilute mixture of boron nitride [3] and water. This was followed by an air bake at 125 °C for several hours to cure the coating, and after the final connection to the embedded sensor, a 4-6 hour 600 °C bake in a vacuum chamber whose base pressures reached the low 10^{-6} torr range by the end of the bake procedure. This coating of boron nitride provided protection to the glass fiber insulating jacket of the signal cable and increased its electrical insulating properties.

IV. Small 1D and 2D Mirnov Coils

Miniature 1-dimensional (1-D) and 2-dimensional (2D) magnetic pickup coils ("Mirnov Coils") for sensing flux changes in one or two directions were fabricated for operating in the thin Center Stack tiles at 600 °C. Ceramic coated wire [4], consisting of AWG No. 36 Kulgrid wire (27% Ni/Cu) and clad with a 0.013 cm (0.0005") layer of

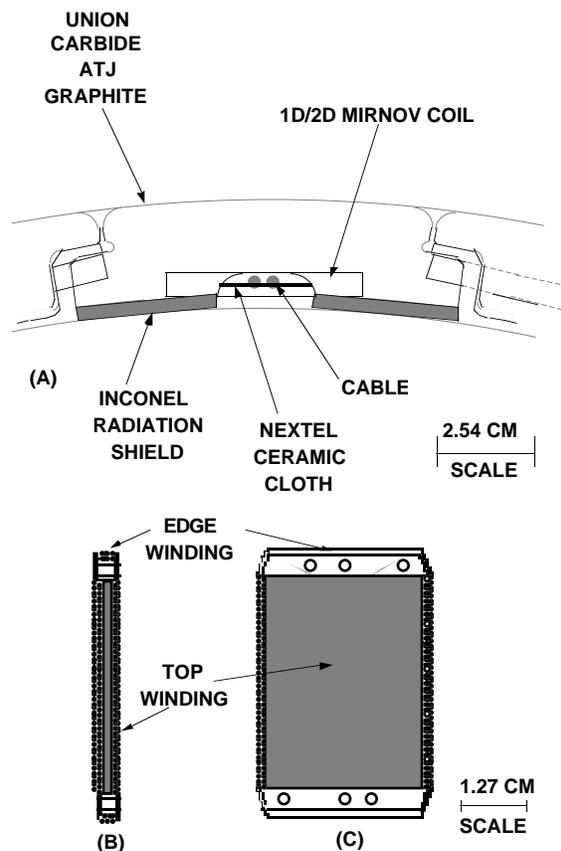


Fig.4. Partial schematic diagram of (a) miniature 1D/2D magnetic sensor coil (Mirnov Coil) installed in 1.27 cm (0.5") thick Center Stack graphite tile, (b) edge view of 2D coil, (c) plasma facing view of 2D coil.

ceramic was wound [5] on a MACOR [6] machineable glass ceramic coil form (see Fig.4). The same form was used for both 1D and 2D coils. The 1D winding coil consists of 2 layers No.36 ceramic coated wire with 190 turns per layer, and the 2D coils have an additional side winding of 2 layers with 14 turns per layer. The fabrication of the 2D Coils, for example, was particularly challenging due to the small space available for the exiting cables. Special fixtures identical in shape to the rear face of a Center Stack magnetic sensor tile were fabricated for the assembly procedure from commercially available casting material. Each fixture was first covered with a thin layer of standard flexible packaging material (“Saran Wrap”). Two twisted pair Cu-Cu cables baked as described above (Sec. III) were untwisted and placed into the channel of the cast. An assembled 2D Coil was placed over the wires, and Omegabond-700 [7] ceramic adhesive was used to fix the wires and coil. The assembly was then removed from the coil form for welding of the No. 24 Cu-Cu wires to the No. 36 wire wound on the coil form. After welding, the coil with attached cables was placed into the recess machined in the rear-face of a Center Stack tile and bonded at 4 points with Omegabond-700 ceramic adhesive. Nextel ceramic cloth tape [8], 0.051 cm (0.020”) thick was placed over the coil and bonded to the coil and wires with Omegabond-700 ceramic adhesive [7]. In some instances, if the close tolerances did not permit the use of the Nextel cloth, then only a layer of Omegabond-700 was applied. The initial curing process was performed at room temperature. The final step in the curing process was an air bake at 200 °C for about 2 hours. The 2D Mirnov Coils for the thicker inner divertor tiles were fabricated in the same manner.

V. Thermocouples

Type-K, AWG No. 24, twisted pair, thermocouple wire [2] with 650 °C temperature rating was cut into units 3.7 m (12') long, stripped of insulation at one for a distance of 2.5 cm (1”) and welded together to form a thermocouple junction about 0.102 cm (0.040”) in diameter. After

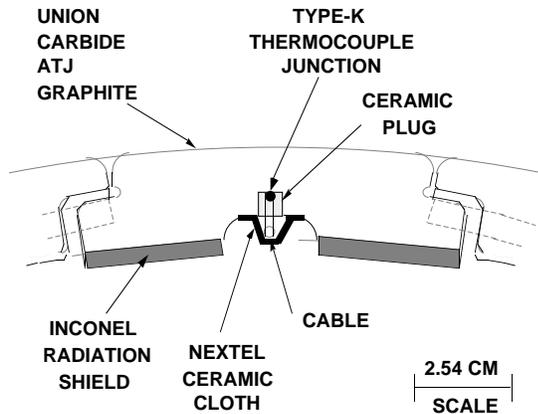


Fig.5. Partial schematic diagram of Type-K thermocouple mounted in 1.27 cm (0.5”) thick Center Stack graphite tile.

welding, the thermocouple unit was air-baked, and then the junction was placed into a hole (“well”) machined into the rear-face of a Center Stack tile. The thermocouple well is 0.318 cm (0.125”) inside diameter by 0.318 cm (0.125”) deep, which positioned the thermocouple junction 0.635 cm (0.25”) from the front face of the tile (Fig.5). A small bend radius was placed in the wire to allow for the 90° transition from the well to the cable channel in a manner that provided a small spring tension to press the junction against the base of the well. Omegabond-700 [7], a high temperature ceramic cement was placed into the well to a height of about 50% of the well depth. This bonded the thermocouple into the well, and effectively created a molded ceramic plug *in situ*. Nextel ceramic cloth [8], 0.051 cm (0.020”) thick by about 2.5-3.18 cm (1-1.3”) long was cemented in the cable channel over the exiting thermocouple wires to press the junction into the well during the curing process, and to provide strain relief for the wires. The width of the Nextel cloth was dimensioned so that it followed the contours of the channel but did not protrude beyond the channel. A weight was placed over the Nextel and thermocouple wires during the curing process at room temperature. The final step in the curing process was an air bake at 200 °C for about 2 hours. The thermocouples for the thicker inner and outer divertor tiles were fabricated in the same manner.

VI. Langmuir Probes

Small plasma probes (Langmuir Probes) were designed to be mounted flush to the front face of selected Center Stack and Divertor tiles. Each Langmuir Probe consists of a 2 mm diameter ATJ graphite probe tip insulated from the surrounding graphite tile by alumina insulators (Fig.6). Two twisted pair Cu-Cu cables baked as described above

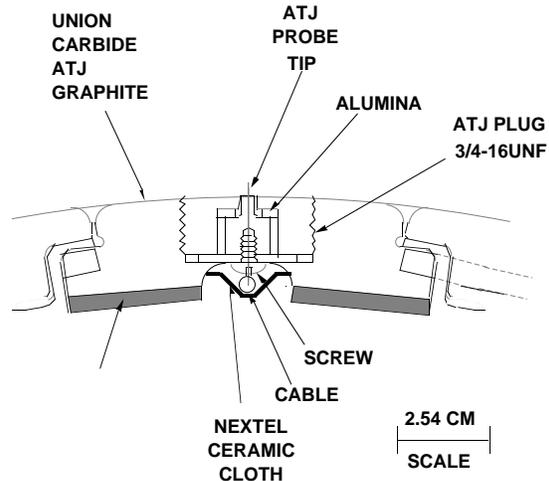


Fig. 6. Partial schematic of a diagram of flush mounted Langmuir Probe in 1.27 cm (0.5”) thick Center Stack graphite tile.

(Sec. III) were welded to a head of a small screw. Thus, the screw head is connected to two wires for redundancy. The screw with the attached twisted pair cable was inserted into the probe tip, and the cable placed into the cable channel. A small amount of Omegabond-700 was placed over the welded junction of the cable and screw for strain relief. As in the case of the thermocouple assembly described above, Nextel ceramic cloth [8], 0.051 cm (0.020") thick by about 2.5-3.18 cm (1-1.3") long was cemented in the cable channel over the exiting Langmuir Probe wires to provide strain relief for the wires. The width of the Nextel cloth was dimensioned so that it followed the contours of the channel but did not protrude beyond the channel. A weight was placed over the Nextel and exiting wires during the curing process at room temperature. The final step in the curing process was an air bake at 200 °C for about 2 hours. The Langmuir Probes for the thicker inner divertor tiles were fabricated in the same manner.

VIII. Large 1D Mirnov Coils

There is a Passive Plate section between each of 12 bays (Fig.1). Each section is separated by a 5.08 cm (2") gap. A poloidal array of large 1-dimensional (1D) magnetic sensors ("Mirnov Coils") was mounted in this gap at one toroidal location. These Large 1D Mirnov Coils consist of two layers of 55 turns each, of AWG No. 26 ceramic wire [4] wound a MACOR [6] mandrel. The outside dimensions of the mandrel are 4.495 cm x 3.493 cm x 1.270 cm (1.770" x 1.375" x 0.5"). The ceramic wire is covered Nextel-312, 2.54 cm (1") wide ceramic tape [8] bonded to the coil with Fortafix Fiborclad high temperature adhesive cement [10] and secured with 0.051 cm (0.020") ceramic thread [11]. Fig.7c show the details of the termination procedure for connecting the coil wire to the exit cables. The cables were clad with fiberglass sleeving [9] for the path to the electrical feedthroughs.

IX. Rogowski Coils

Rogowski Coils are mounted around a conducting medium and measure the enclosed current. Inside the NSTX vessel, 4 Rogowski Coils are mounted around the Center Stack to measure plasma induced halo currents in the Center Stack. In addition, at present, 5 Rogowski Coils are mounted to measure the eddy currents induced in the lower Passive Plate supports. These are mounted so as to provide a toroidal array and a poloidal array at one lower vessel toroidal location. Eventually, depending on work in progress, there may be a total of 16 Rogowski Coils, a set of 4 coils, one on each Passive Plate element, at 4 toroidal locations. The in-vessel Rogowski Coils required special development in order to accommodate the required bend radii, small space limitations using relatively inflexible ceramic materials. A

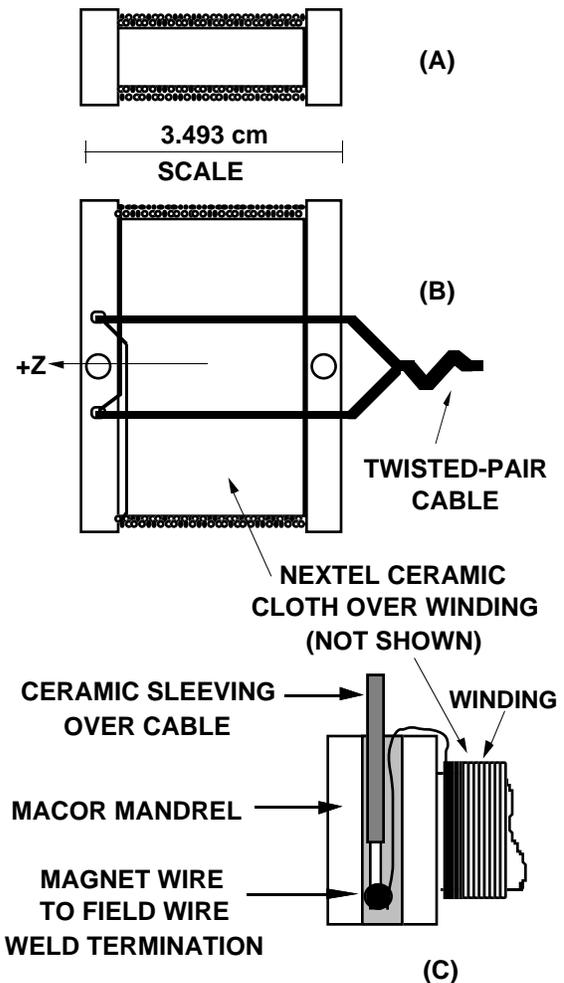


Fig.7. Partial schematic diagram of Large 1D Mirnov Coil magnetic sensors, (a) end view, (b) plasma facing view, (c) expanded detail of winding connection to cabling.

detailed description of this design is given in an associated paper in these Proceedings [12].

VII. Toroidal Flux Loops

Flux Loops were installed on the air-side of the Center Stack (Table 1). These consisted of Teflon insulated AWG No. 22 copper wire (220 °C rated) cemented in place with Omegabond-700 [7]. Inside the vessel (Fig.1), there are Flux Loops mounted under the upper and lower divertors, behind the copper Passive Plates, and on the inner outer wall. These Flux Loops consist of the same Cu-Cu twisted pair wire described above and were baked in the same manner (Sec. III). This twisted pair wire was inserted into thin wall 0.025 cm (0.010"), 304-SS tubing. Hence, for redundancy, each Flux Loop tube has two wires that encircle

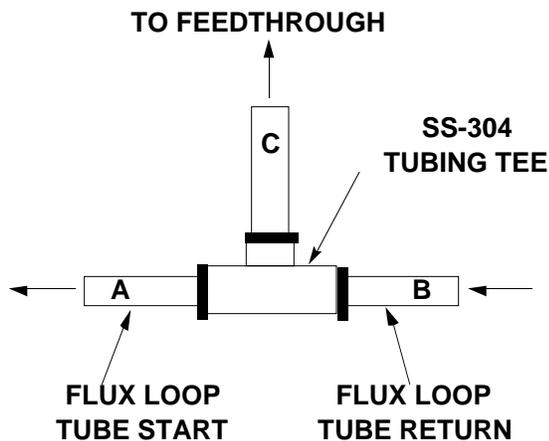


Fig.8. Partial schematic diagram of Flux Loop Tee-section which joins the ends of the flux loop and provides a conduit to the electrical feedthrough. The main toroidal tube (a and c) is 0.476 cm (3/16") O.D. and the conduit to the feed through (c) is 0.635 cm (1/4") O. D. for the Passive Plate Flux Loops.

the torus and are individually connected to electrical feedthroughs. In the case of the Flux Loops mounted on the inside of the outer wall, the tubing outside diameter is 0.635 cm (0.25"). The tubing for all of the other interior Flux Loops had a smaller outside diameter of 0.476 cm (0.188") due to space limitations. Standard 304-SS tubing Tees were used to join the ends of each Flux Loop C-section and provide an exit channel for the cabling to the electrical feedthroughs. The output of a particular Tee unit was coupled to either another 304-SS tube which served as a conduit for the exiting cable, or depending on accessibility, a 650 °C Markel Thermoflex-1200 fiberglass sleeving [9] was used.

X. Electrical Feedthroughs

The vessel internal hardware will be bakeable to 350 °C. The outer vessel port covers will be cooled during bakeout to 150 °C. The electrical feedthroughs must accommodate the 150 °C temperature of the port flange and any additional radiative heating from nearby hardware at a higher temperature. The feedthroughs used for the Center Stack sensors are standard 19 pin double ended Ceramaseal [13] connectors for the Cu-Cu cables, or 10 pin thermocouple double ended connectors as required. The feedthroughs used for the outer vessel sensors are standard 32 pin double ended Ceramaseal [13] connectors for the Cu-Cu cables, or 20 pin thermocouple double ended connectors as required. The cables are stress relieved at the Center Stack feedthroughs by enclosing the cables in a sleeving fabricated from Nextel-312 [7] and fastened with ceramic thread [11]. The cables are stress relieved at the outer vessel feedthroughs using ceramic thread to fasten the cables to a

304-SS rod protruding into the vessel from the inside face of the port flange near the feedthrough.

XI. Conclusions

The design of the more than 300 in-vessel sensor systems for the National Spherical Torus Experiment (NSTX) has encountered several challenging fusion reactor diagnostic issues involving high temperatures and space constraints. This has resulted in unique miniature, high temperature in-vessel sensor systems mounted in small spaces behind plasma facing armor tiles, and they are prototypical of possible high power reactor first-wall applications.

Acknowledgments

We acknowledge the technical contributions of M. Anderson, J. Bartzak, W. Derry, S. Edwards, G. Gibilisco, K. Gilton, S. Jurcznski, P. Kivler, R. Knolls, G. Rossi, F. Simmons Jr., S. Vinson, and J. Winston. Work Supported by USDOE Contract No. DE-AC02-76-CHO3073

References

1. S. M. Kaye et al., "Physics Design of the national Spherical Torus Experiment", *Fus. Technol.* **36**(1), 16 (1999).
2. Thermo Electric Co., 100 North Fifth Street, Saddle Brook, NJ, USA.
3. Carborundum Co., Boron Nitride Division, Audubon Industrial Park, Amherst NY 14228-2027, USA.
4. Ceramawire, P.O. Box 2597, Elizabeth City, NC 27908-2597, USA.
5. Airex Corp., Route 108, Dover, NH 03820, USA.
6. MACOR, Corning Materials Business, Corning Glass Works, Corning, NY, 14830, USA.
7. OMEGA Engineering Corp., One Omega Drive, P. O. Box 4047, Stamford, CT 06907-0047, USA.
8. Nextel (Trade Mark, 3M Co.) Fiber Materials, Inc. 5 Morin Street, Biddeford, ME 04005-4497, USA.
9. Markel Corp. P.O. Box 752, Norristown, PA, USA.
10. Fortafix Inc. First Drove, Fengate, Peterborough, PE1 5 BJ, England.
11. Cotronics Corp., 3379 Shore Parkway, Brooklyn, NY, 11235, USA. #391T-10 ceramic thread
12. B. McCormack, *et al.*, "Rogowski Loop Designs for NSTX", in these Proceedings.
13. Ceramaseal, Inc., P.O. Box 260, Route 20, New Lebanon, NY 1215, USA.